

An Efficient Approach for Ultrasonic Characterization of Biomaterials using NI Lab VIEW

Arun V. Padole¹, Y.B. Gandole²

¹Research Student, Department of Electronics, Adarsha Science J.B. Arts and Birla Commerce, Mahavidyalaya Dhamangaon Railway, Dist. Amravati- 444 709 , India.

²Department of Electronics, Adarsha Science J.B. Arts and Birla Commerce, Mahavidyalaya Dhamangaon Railway, Dist. Amravati- 444 709, India.

ABSTRACT: The methodology for characterization of biomaterial is the source of signal, Biomaterial and the response detector. The high frequency ultrasonic signal generator generates signals of high frequency suitable for biomaterial characterization. In this system, Ultrasonic signals are made to fall on the biomaterial to be characterized. While passing through the biomaterial, the ultrasonic signals are absorbed, reflected and scattered along different directions. The transmitted and reflected received signals are sense and detect by receiving transducer. The sensor produces proportional current in microamperes. This current will be applied to sensing circuit, which converts current into proportional amplified voltage with the help of Op-Amp. An Analog to Digital Converter (ADC) converts analog signal into digital signal. This digital signal provides data to a computer. Data acquisition circuit interconnects the PC and driver software to which the data is input. Driver software makes NI LabVIEW to interact with hardware. The PC with LabVIEW platform is used to study characteristics of the biomaterials.

Keywords: Attenuation, Biomaterial, LabVIEW, Ultrasonic signals, Velocity

I. INTRODUCTION

The ultrasonic NDT technique is a versatile tool for the characterization of material. The main objective of this NDT technique is to certify that the sample material being examined is fit for the intended service. Ultrasonic investigation in biomaterials relies mainly on the study of behavior of wave propagation. Ultrasonic velocity and attenuation measurements can be computed in biomaterials by knowing the distance and time of flight.

The present study represents, Virtual Instrumentation system using NI LabVIEW for the biomaterial characterization. The work describe here is carried out to improve accuracy, precision, reliability of ultrasonic velocity and attenuation measurement in solid biomaterials, as well as to fulfill the need of biomedical industry so as to enhance the patient's quality of life. The developed system is dedicated for the measurement of ultrasonic velocity and attenuation relative to evaluation of properties for the biomaterials Aluminum, Copper, 316L Stainless steel, Cast Iron.

The ultrasonic velocity is very useful for determining several important material parameters like porosity, residual stresses, texture and characterization of secondary phases in microstructure. In order to study the small and important variations, high-resolution technique for ultrasonic velocity measurements are necessary [1].

1.1 Virtual Instrumentation

Virtual instrumentation uses mainstream computer technology combined with flexible software and high performance hardware technology to create powerful computer based instrumentation system. The objective in Virtual Instrumentation is to use a PC to mimic real instrument with their dedicated controls and displays with the added versatility that come with software. Virtual Instrumentation combines hardware and software with computer technology to create user defined instrumentation system.

Virtual instrument is an effective and powerful combination of hardware and software. It combines processing power of PC with flexible software for numerous measurements. Engineers and scientist can create user defined systems to meet their exact application needs. The virtual instrumentation can be realized using software like LabVIEW, VB, JAVA etc and DAQ card as per the application. LabVIEW (Laboratory Virtual Instrument Engineering Workbench) is a graphical programming environment language to design virtual instrument [2].

Manual analog methods used for measurements are tedious and time consuming. Thus without computer automation the necessary measurements for material property evaluation would certainly be impractical where speed, accuracy and economy is required [3].

The ultrasonic velocity measurements using the present PC based system are found to be precise and consistent. The instruments that were used for ultrasonic measurements are replaced by Virtual Instrumentation [4]. A virtual design and testing procedure can save time and money [5].

1.2 NI LabVIEW 2010

LabVIEW is an integral part of Virtual Instrumentation because it provides an easy-to-use application development environment designed specifically for engineer and scientist. LabVIEW offers powerful features that make it easy to connect to wide variety of hardware and software. One of the most powerful features that LabVIEW offers is graphical programming language.

Laboratory Virtual Instrument Engineering Workbench (LabVIEW) is a graphical programming language written by National Instruments for the development of acquisition software that uses icons instead of lines of text to create programs. Its graphical nature makes it ideal for test and measurement, data acquisition, data analysis and instrument control applications. This results in significant result improvements over conventional programming languages. LabVIEW is an entirely graphical paradigm with the concepts of the block diagram and the front panel. LabVIEW, as a programming language, is a powerful tool that can be used to achieve our goals [6].

1.3 Ultrasonic attenuation and velocity in materials

Ultrasonic attenuation, velocity and their related parameters can be used to give insight into materials microstructures and associated physical properties. Behavior of ultrasonic attenuation and velocity as a function of physical parameters related to different physical condition is used to characterize the material during the processing as well as after production [7].

Velocity: To measure the ultrasound velocity in the sample, the formula is given by:

Velocity = Distance / Time

Where 'T' is the time elapsed between registering echoes [8].

The ultrasonic velocity is calculated by knowing the distance between the two parallel external surfaces of the sample in which wave travel, hence

Velocity = Thickness / Time (m/sec) [9].

Some of the non-destructive testing techniques, which have been used to characterize material properties, are ultrasonic testing, radiometry, magnetic methods, eddy current testing, Barkhausen noise, Mossbauer spectroscopy etc. Ultrasonic Testing is the most preferred NDT technique for characterization of material properties [10].

For the measurement of ultrasonic velocity and attenuation in materials a number of techniques are used. Some of the standard techniques used for the measurement of ultrasonic velocity are: pulse-echo technique, sing-around technique, diffraction technique and interferometer technique. The sing-around technique is more accurate for measurement of ultrasonic velocity. This can be described by Soitkar et.al. [11] and Beyer et al. [12]. The ultrasonic pulse-echo overlap technique is widely used for the ultrasonic velocity measurement, as it is accurate and versatile by Papadakies [13], Hellier et al. [14]. They also presented the circuits of pulse-echo-overlap technique.

Now a day's several new pulse techniques, with extremely high degree of precision have been developed for ultrasonic measurements. A solid-state variable frequency pulser-receiver system has been developed by Yawale et al. [15]. A solid-state pulser-receiver system for ultrasonic velocity measurement at fixed frequency using digital circuitry has been developed by Agnihotri et al. [16].

1.4 Biomaterials

The materials which are used for structural applications in the field of medicine are known as Biomaterials. These materials are successfully used to replace damaged parts in human or animal bodies. These materials are able to function by remaining in intimate contact with the living tissues, with a minimum adverse reaction to the body. Sometimes, a single material cannot fulfill the complete requirement of specific application; in that case, a combination of more than one material is used. In ancient times, metals were used for orthopedic applications. Pure metals such as Silver, Gold and Copper were used for different medical applications. In view of requirements of suitable materials for medical applications, the alloys such as 316L Stainless Steel and Ti-6Al-4V have been developed for orthopedic applications [17].

The biomaterials used in our experiment are given below,

- a) Aluminium.
- b) Copper.
- c) Stainless Steel 316L
- d) Cast Iron

1.5 Basics of the System

In this system procedure is intended for 20 mm thick solid biomaterials. The surface is kept parallel to the direction of energy propagation and has been maintained parallel to at least 10°. Several possible modes of vibration can propagate in solids. This procedure is concerned with velocity of longitudinal wave. The longitudinal velocity is independent of sample geometry when the dimensions at right angles to the beam are very large compared with beam area and wave length.

The ultrasonic testing system to be used in this work shall include the following apparatus.

1.5.1 Test Instrument—an ultrasonic instrument comprising a transmitter, receiver, and a data acquisition circuit to generate, receive, and display electrical signals related to ultrasonic waves. The equipment allows readings for the positions of 80mm & 180mm.

1.5.2 Search Unit— the search unit containing a transducer that generates and receives ultrasonic waves of an appropriate size, type and frequency, designed for tests by the contact method shall be used. Contact straight beam longitudinal mode shall be used for longitudinal velocity measurements. Here we make use of a 5MHz transducer.

1.5.3 Couplant – for longitudinal velocity measurements, the clean light –grade oil can be used as Couplant [18].

II. INSTRUMENTATION

2.1 Working Principle

The frequency generator circuit generates a signal of 5MHz frequency. This signal is fed to transmitting transducer which is at one end of the measuring cell. At the same time in microcontroller system, controller generates the trigger with specific time & amplitude, this trigger goes on vary with respect to time & amplitude till receiver will not receive the signal. The trigger time & amplitude will be variable for different sample. As soon as the signal is received by the receiving transducer at another end the system measures the peak amplitude of T_x & R_x signal. This process will be carried for multiple attempts. In single attempt, wave count is also measure with respect to transmission, reception and hence also wave drop. Finally controller measure transition time for the wave. All these data will be recorded in DAQ for future use and to transmit to PC.

2.2 System Block Diagram

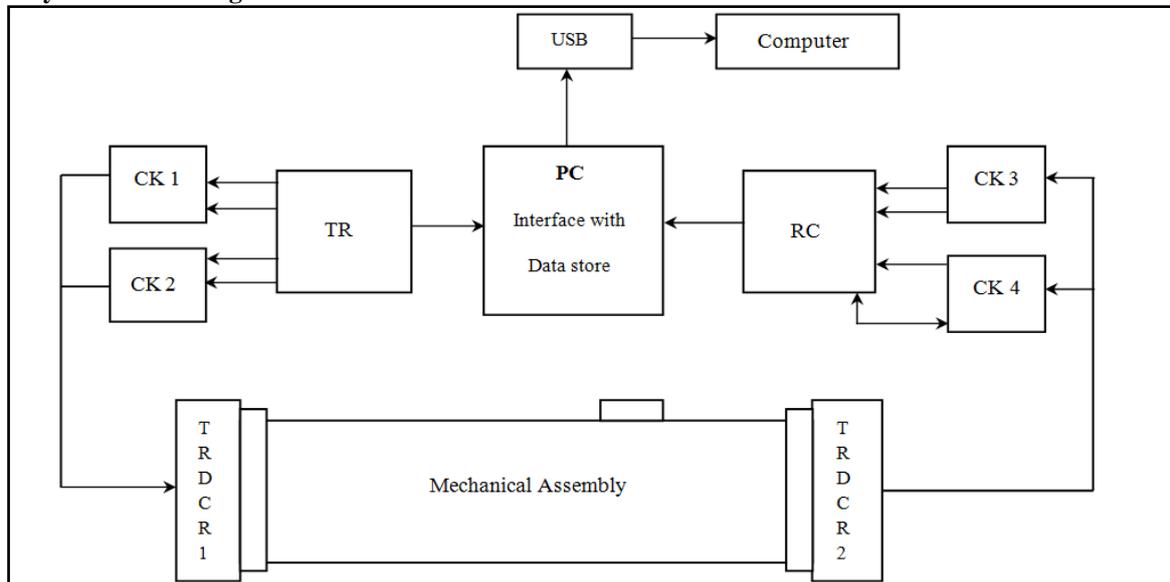


Figure 1: System Block Diagram

2.3 Block Diagram Description

The block diagram of the system is shown in Fig.1. The system consists of mechanical assembly embedded with a transducer pair. Receiver-transmitter circuits are also shown in support of two separate circuits each. Circuit 1 and circuit 3 are filter amplifier circuits while circuit 2 and circuit 4 are signal conditioner for the same. Receiver-Transmitter PCB's are interlinked to master PCB. Master controls all the triggering actions and also works for the data collections from the sub-circuits. Finally master interlinks the PC via USB driver as a part of data acquisition for virtual instrumentation for connectivity to Lab VIEW.

At the other end of biomaterial sample the receiver circuit receives, modulates and filters the received ultrasonic signal. First amplification of the signal is performed then two stage filters removes the unwanted transients and finally this signal will be send to data acquisition device.

IV. MEASUREMENT TECHNIQUE

For the measurement of ultrasonic velocity and attenuation, the transmitting transducer is firmly fixed at one end of the measuring cell while receiving transducer is fixed to movable end. The biomaterial sample is placed between two transducers. The ultrasonic velocity and attenuation measurements can be Computed and displayed on personal computer.



Figure 4: Measuring cell with associated circuit

Block Diagram: The block diagram contains graphical programming code as shown in Fig. 5. .

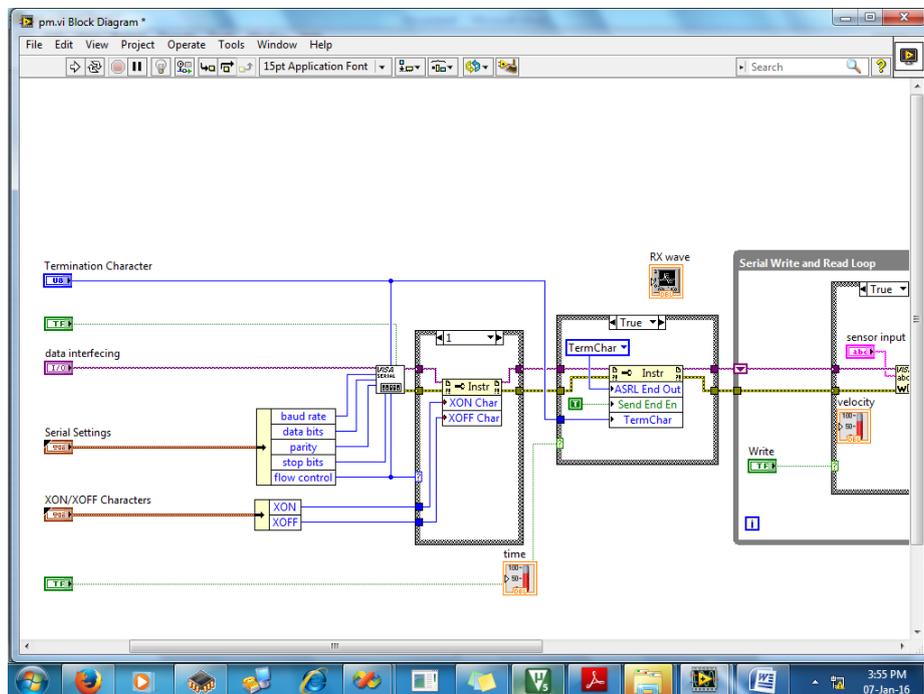


Figure 5: Screen shot showing the block diagram of the project

Front Panel: All input and output status are available on front panel as shown in following Fig. 6.

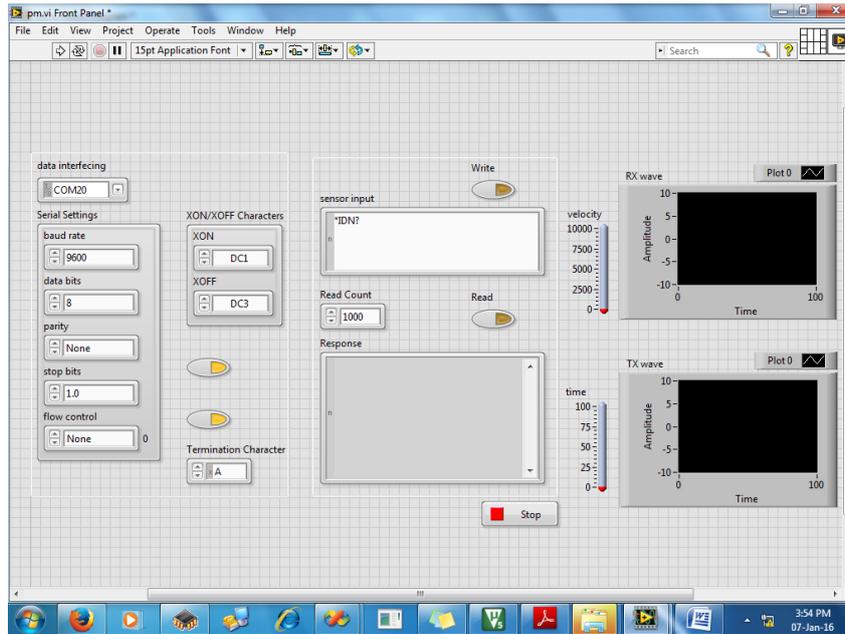


Figure 6: Screen shot showing the front panel of the project

V. RESULT AND DISCUSSIONS

The system is checked by measuring the ultrasonic velocity and attenuation in different biomaterial samples at 5 MHz frequency. The distance between transmitting transducer and receiving transducer is kept 80mm and 180mm. Table 1: shows the comparison between the literature/ theoretical values and experimentally observed values of ultrasonic velocity in the biomaterial samples.

Table 1: Ultrasonic velocity measurement at 5MHz

Velocity									
Element	d=180mm		d=80mm		Velocity(m/S)		Deviation		Average % Deviation
	Avg. time	Velocity (m/S)	Avg. time	Velocity (m/S)	Observed (Avg)	Theoretical	Value	Percentage	
Aluminium	28.51	6312.84	12.65	6324.11	6318.47	6300.00	-18.47	-0.29	0.07
SS316L	30.43	5915.86	13.62	5875.15	5895.51	5900.00	4.49	0.08	
Coppr	38.41	4685.87	17.12	4672.90	4679.39	4700.00	20.61	0.44	
CastIron	42.74	4211.18	19.12	4183.37	4197.28	4200.00	2.72	0.06	

The theoretical (literature) values are referred from the reference [18].

Graphs:

The graphs shown in Fig.7 are obtained from observation table.

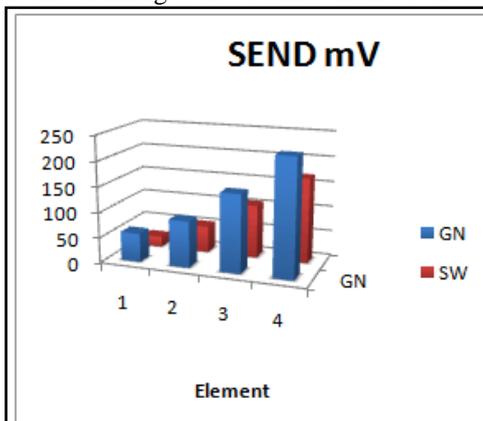


Figure 7: Graph between biomaterial elements and average sending signal amplitude.

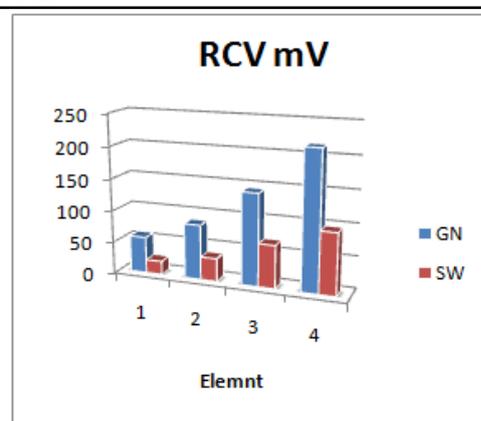


Figure 8: Graph between biomaterial elements and average signal received amplitude.

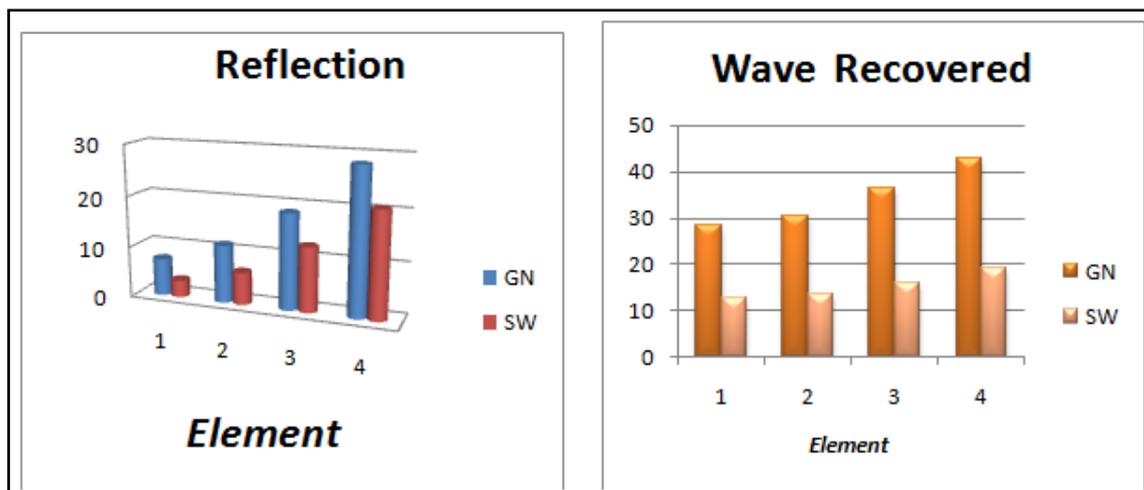


Figure 9: Graph between biomaterial elements and reflections.

Figure 10: Graph between biomaterial elements and wave recovered.

VI. CONCLUSIONS

From the table 1, it is observed that, the experimental values of ultrasonic velocity and attenuation at 5MHz frequency are in good agreement with the literature values. Moreover, it shows a very small deviation in the observed values, which signify the high accuracy, precision, reliability of the system. Hence it is conclude that the developed Virtual Instrumentation system shows good performance and can be used for the characterization of biomaterials.

REFERENCES

- [1] Shaik Abdul Jaffar, K. Malakondiah and Y. B. Gandole (2012). Design and Development of Computer Based Ultrasonic Velocity Measurements in Liquids. International Journal of Power System Analysis, ISSN: 2277-257X, Vol: 1, No: 2 pp 38-44.
- [2] A.C. Balharpure, A.S. Pande, S.J. Sharma and Rajagopalan, "Design of LabVIEW Based Virtual Instrument for Sing around Technique", International Journal of Engineering Research and applications (2014), pp 37-42.
- [3] NASA Technical Memorandum 79180, Alex Vary Lewis Research Centre Cleveland, Ohio 44135, "COMPUTER SIGNAL PROCESSING FOR ULTRASONIC ATTENUATION AND VELOCITY MEASUREMENTS FOR MATERIAL PROPERTY CHARACTERIZATION", (1979), PP 1-11.
- [4] Rajagopalan S., Sharma S. J. & Ghodki V. M., "Low cost virtual instrumentation using PC printer port for ultrasonic velocity measurements", Electronic Journal <<Technical Acoustics>> 2007, 12 pp 1-8.
- [5] Gandole Y.B., "Computer Modeling and simulation of Ultrasonic Signal Processing and Measurements", Hindawi Publishing Corporation Physics Research International, Volume 2012, pp 1-12.
- [6] HPK Kumar, (2008-09). VI Based Temperature sensing and controlling using NI LabVIEW. pp 01-53.
- [7] Pandey D. K. (September 2010). Ultrasonics: A Technique of Material Characterization. pp. 466.
- [8] Dr. Kailash and Shri K. S. Kushawaha, "Ultrasonic Techniques for Measurement of Propagation Parameters", 2001, pp 90-123.
- [9] Golhar A.R., Sawadh P.S. & Choudhari N. K., "Simulation Technique Used to Evaluate the Characteristic of Aluminium Metals by Ultrasonic Non-Destructive Techniques", Indian Journal Of Applied Research, Volume 3 , Issue 9 Sept. 2013, pp 198-200.
- [10] Nanekar P.P. & Shah B.K. "Characterization of Material Properties By Ultrasonics", BARC Newsletter, Issue No. 249, pp 25-38.
- [11] Soitakar V.S., Navaneet G.N. and Sunnapwar "Receiving system design for sing around technique in ultrasonic measurements", Indian J. Tech.,(1980), pp 18,469.
- [12] Beyer R.T. and Letcher S.V. "Physical ultrasonic", Academic press, New York,(1969),pp 87.
- [13] Papadakis p, New, "compact instrument for pulse echo overlap measurements of ultrasonic wave transit times", Rev Sci. Instrum, (1976), pp 47, 806.
- [14] Hellier A.G., Palmer S.B. and Whitehead D.G. "An integrated circuit pulse echo overlap facility for measurement of velocity of sound", Journal of Physics E: Scientific Instruments, (1975), Vol 8, pp 352-354.
- [15] Yawale S.P. and Pakade S.V. "Solid state variable frequency pulser -receiver system for ultrasonic measurements", Indian Journal of pure and Applied Physics.,(1995), Vol 33, pp 638-642.
- [16] Agnihotri P. k. and Adgaonkar C. S. "Theoretical evaluation of Ultrasonic velocity in binary liquid mixtures", Research and Industry, (1988), pp 33,139.
- [17] Rajendran V., Marikani A., "Materials Science", 'Biomaterials', Fifth Reprint 2006, TMH, pp 22.1-22.5. ISBN: 0-07-058369-2
- [18] ASTM, "Standard Practice for Measuring Ultrasonic Velocity in Materials", an American National Standard Designation: E 494-95, March 1995, pp 1-14